



The ShurFit LLIF interbody design provides six footprints with a parallel and 7° lordotic angle to assist in reproducing the patient's sagittal profile while providing anterior column support.

- The Large Graft Window optimizes biological ingrowth
- The Self-distracting Bulleted Leading Edge allows for easy insertion
- Sizing
 - Lordosis – 0 & 7 Degrees
 - Width – 18 & 22mm
 - Height – 8, 10, 12, 14 & 16mm



Bulleted
Leading Edge



The AccuFit® Lateral Plate features a low profile design with five lengths (30, 32, 34, 36, & 38mm lengths). The system also features a unique, plate placement locking guide for easy screw insertion.

- Double Lead Screw provides efficient delivery
- Retention Driver allows for secure screw placement
- Variable Angle Plate provides optimal screw placement
- Screw Sizing
 - Diameter 5.5 & 6.5mm
 - Length 30-60mm (5mm inc.)





AnyPlus[®] TLIF CAGES

A comprehensive system
for transforaminal lumbar
interbody fusion

KEY FEATURES & BENEFITS

MULTIPLE FOOTPRINTS

- Three lordotic options in multiple heights and lengths conform to varying patient anatomies

ANATOMICAL DESIGN

- Provides optimal contact with the vertebral endplates, minimizing potential implant subsidence

BULLET-SHAPED LEADING EDGE

- Facilitates ease of insertion

AGGRESSIVE TOOTH PATTERN

- Provides stability and reduces the risk of implant migration

LARGE GRAFT FENESTRATIONS

- Allows for a higher volume of bone grafting material resulting in good bony ingrowth

MATERIAL PROPERTIES

- Cages are manufactured from PEEK-OPTIMA[®] a biocompatible, radiolucent polymer that enhances visualization of bone growth in and around the implant
- Embedded tantalum markers facilitate intraoperative placement and radiographic confirmation of implant position

OPERATIVE FLEXIBILITY

- Articulating inserter allows for implant manipulation within the disc space

HIGH-QUALITY
COST-EFFECTIVE
SURGICAL SOLUTIONS



AnyPlus®
TLIF CAGES



A versatile system that enables a bilateral, unilateral or transforaminal approach to the vertebral bodies.

Simple and intuitive instrumentation facilitates easy cage insertion.



AnyPlus® TLIF Cages

Included in TLIF set

		9 mm width									
		Height (mm)									
Lordosis / Length (mm)	0°	7	8	9	10	11	12	13	14	15	16
	28										
	31										
	4°	28									
	31										
	7°	28									
	31										

		11 mm width									
		Height (mm)									
Lordosis / Length (mm)	0°	28									
	31										
	4°	28									
	31										
	7°	28									
	31										

GSMedicalUSA.com

GS Medical

866.904.8144

5200 SOQUEL AVE, STE 104
SANTA CRUZ, CA 95062 U.S.A.

GS100-105-LIT


PRECISION SPINE

SHURFIT®

INTERBODY CAGES

PATIENT MATCHING OPTIONS

The ShurFit family of interbody cages includes designs for T-PLIF, PLIF and TLIF procedures. The ShurFit designs offer a large contact area to optimize vertebral body support and minimize possible risk of subsidence. The large graft window allows for maximum biological coverage area for fusion. Simple instrumentation offers ease of implantation for surgeons, while the unique tooth pattern geometry may minimize the potential for expulsion. The PEEK ShurFit Interbody cages are available in multiple sizes to accommodate varying anatomies and effect optimal patient matching.

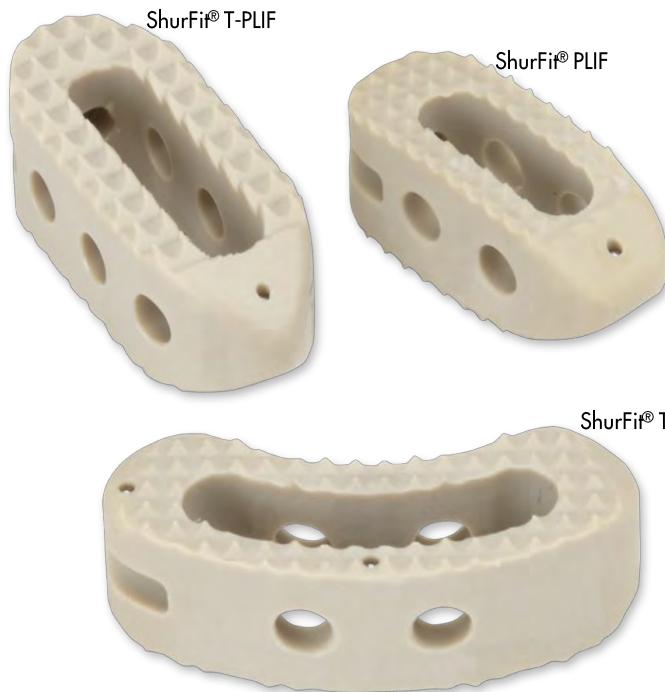


PRECISION SPINE®

Discover the Difference




SHURFIT® INTERBODY CAGES

ShurFit® PLIF Interbody Cages

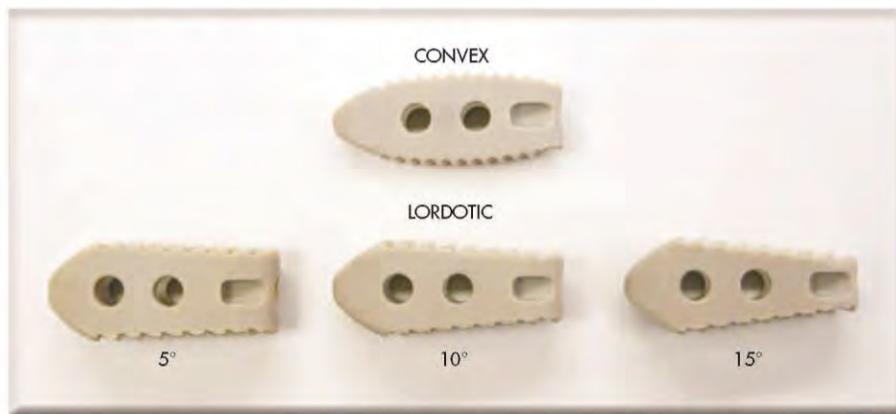


ShurFit® TLIF Interbody Cages

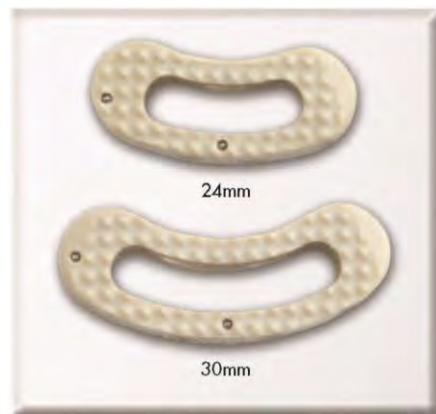

- Large graft window
- Convex & Lordotic Series (Available in 5°, 10° & 15°)
- Bulleted Nose
- 22mm & 25mm Lengths
- 9mm Width
- 8 to 16mm Heights (1mm increments)

- Large graft window
- 24mm & 30mm Lengths
- 9mm Width
- 6 to 16mm Heights (2mm increments)

ShurFit® T-PLIF Interbody Cages

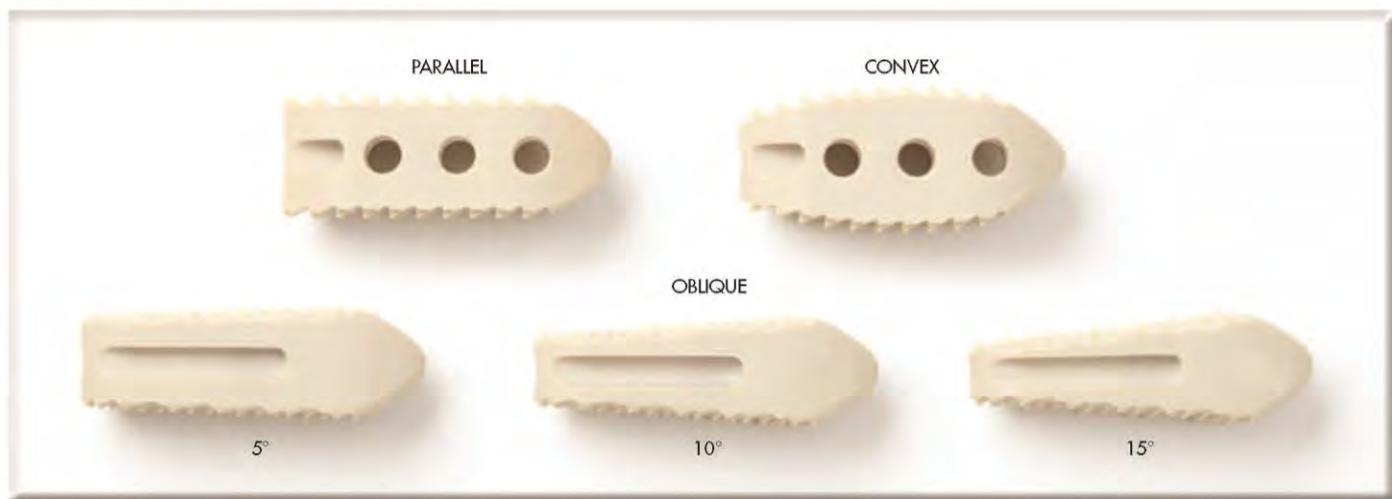

- Large graft window
- Straight and Convex Options
- Bulleted Nose
- 28.5mm Lengths
- 11mm Width
- 7 to 16mm Heights (1mm increments)

Three options from the extended line
of ShurFit Interbody Cages.

Precision Spine, Inc.

2050 Executive Drive, Pearl, MS 39208

Customer Service: 1.888.241.4773

Phone: 601.420.4244

Toll Free: 877.780.4370

Fax: 601.420.5501

www.precisionspineinc.com

Caution: Federal (USA) law restricts these devices to sale by, or on the order of, a physician.

ShurFit® and Precision Spine® are trademarks of Precision Spine, Inc.


Copyright 2020 Precision Spine, Inc. All rights reserved. P/N LBL-FB-002 Rev E 03/2020

PRECISION SPINE®
CE 2797

Twin Peaks TLIF

by SPI

Transforminal lumbar interbody fusion cage Cage de fusion lombaire transforaminale intersomatique Caja de fusión lumbar intersomática transforaminal

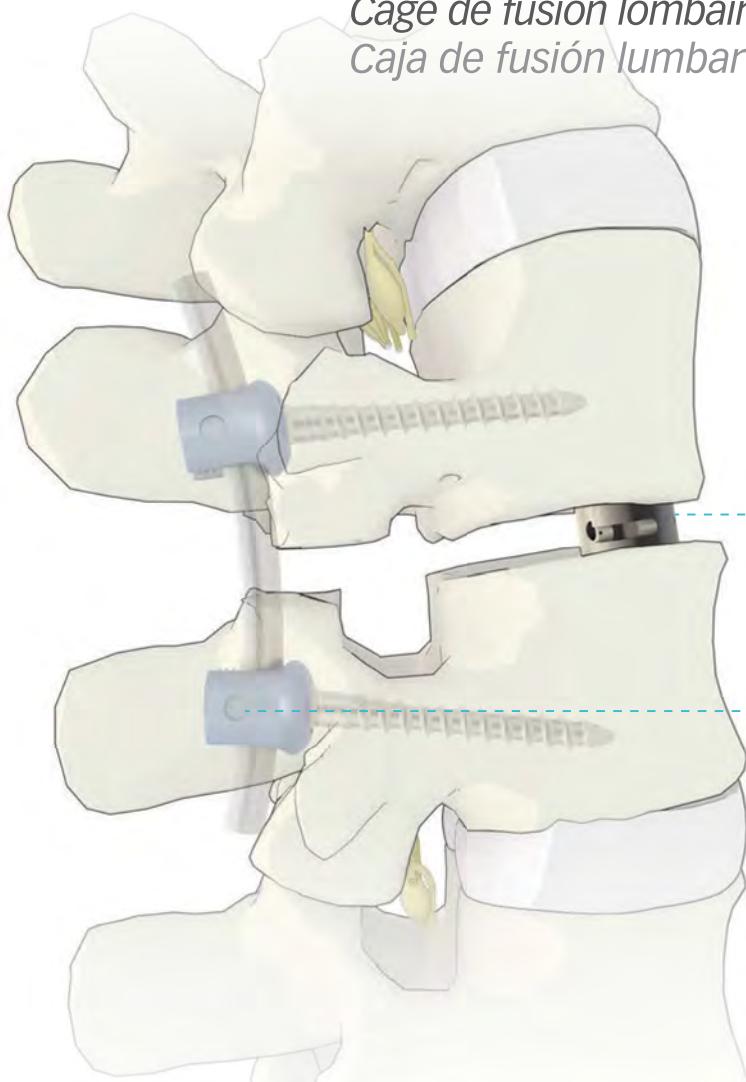

Indications for use

Intervertebral body fusion procedures in skeletally mature patients with degenerative disc disease (DDD) of the lumbar spine at one or two contiguous levels from L2-S1.

For more information, please consult the Twin Peaks TLIF Surgical technique.

Indications

Interventions de fusion intervertébrale chez des patients dont le squelette a atteint la maturité, souffrant de discopathies dégénératives (DDD) de la colonne vertébrale, à un ou deux niveaux contigus, de L2 à S1.

Pour plus d'informations, merci de vous reporter à la technique opératoire Twin Peaks TLIF.



--> **Lumbar cage TLIF**
Cage lombaire TLIF
Caja lumbar TLIF



--> **Sonora or Neve**

OUTSIDE USA:.

sonora : calcium phosphate ceramic granules
neve : hydroxyapatite nanoparticle gel

HORS ÉTATS-UNIS :

sonora : Granules de céramique de calcium phosphate
neve : Gel de nanoparticules d'hydroxyapatite.

FUERA DE EE.UU.:

sonora : Gránulos de cerámica de fosfato de calcio.
neve : Gel de nano partículas de hidroxiapatita

--> **Mont Blanc - Pedicle screw system**

Indicaciones de uso

Procedimientos de fusión de cuerpos intervertebrales en pacientes con esqueleto maduro que padecen enfermedad discal degenerativa (EDD) en la columna lumbar en uno o dos niveles contiguos de L2 a S1.

Para más informaciones, consulte a la Técnica quirúrgica Twin Peaks TLIF.





NEWAY



Implants, supplied sterile.
3 radio-opaque markers.

Implants délivrés stériles.
3 marqueurs radio-opaque.

Implantes suministrados
estériles.
3 marcadores radio-opaco

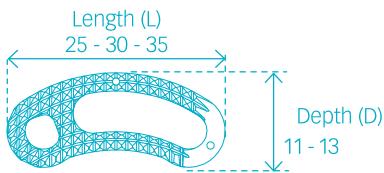

lumbar cages TLIF - cages lombaires TLIF - cajas lumbares TLIF

S

Length 25

$\alpha^{\circ} 4$

Part number	L	H	D	α°
TP1T7254	25	7	11	4°
TP1T8254	25	8	11	4°
TP1T9254	25	9	11	4°
TP1T10254	25	10	11	4°
TP1T11254	25	11	11	4°
*TP1T12254	25	12	11	4°
*TP1T13254	25	13	11	4°

$\alpha^{\circ} 9$

M

Length 30

Part number	L	H	D	α°
TP1T7304	30	7	13	4°
TP1T8304	30	8	13	4°
TP1T9304	30	9	13	4°
TP1T10304	30	10	13	4°
TP1T11304	30	11	13	4°
TP1T12304	30	12	13	4°
TP1T13304	30	13	13	4°
*TP1T14304	30	14	13	4°

L

Length 35

Part number	L	H	D	α°
TP1T7354	35	7	13	4°
TP1T8354	35	8	13	4°
TP1T9354	35	9	13	4°
TP1T10354	35	10	13	4°
TP1T11354	35	11	13	4°
TP1T12354	35	12	13	4°
TP1T13354	35	13	13	4°
*TP1T14354	35	14	13	4°



Materials:

- PEEK OPTIMA® by Invibio®
- Radio-opaque markers: tantalum.

All dimensions are measured in millimeter

*On request, delivery time not guaranteed

Matériaux :

- PEEK-OPTIMA® par Invibio®
- Marqueurs radio-opaques : tantalum.

Toutes les dimensions sont mesurées en millimètres.

*Sur demande, délai de livraison non garanti

Material :


- PEEK OPTIMA® por Invibio®
- Marcadores radiopacos: tantalio.

Las dimensiones se mide en milímetros

*Bajo pedido, plazo de entrega no garantizado

Twin Peaks OLIF

by SPI

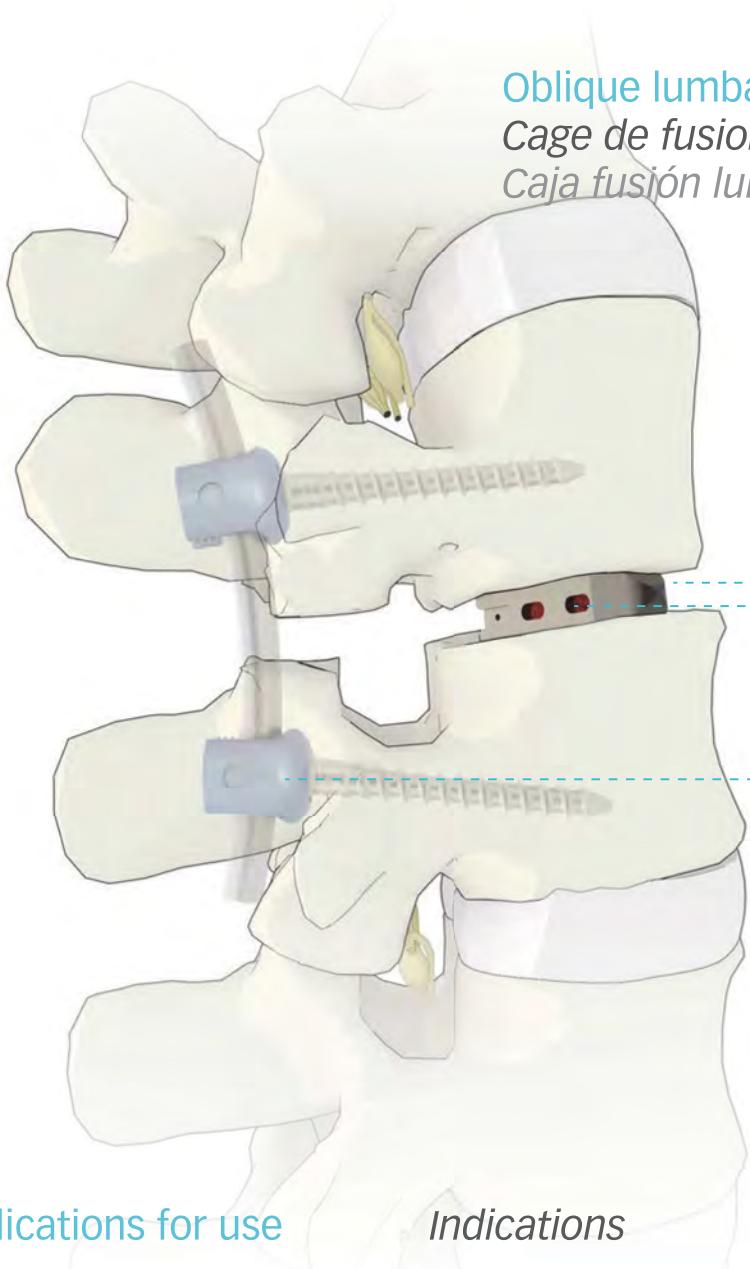

Indications for use

Intervertebral body fusion procedures in skeletally mature patients with degenerative disc disease (DDD) of the lumbar spine at one or two contiguous levels from L2-S1.

For more information, please consult the Twin Peaks OLIF Surgical technique.

Indications

Interventions de fusion intervertébrale chez des patients dont le squelette a atteint la maturité, souffrant de discopathies dégénératives (DDD) de la colonne vertébrale, à un ou deux niveaux contigus, de L2 à S1.


Pour plus d'informations, merci de vous reporter à la technique opératoire Twin Peaks OLIF.

Indicaciones de uso

Procedimientos de fusión de cuerpos intervertebrales en pacientes con esqueleto maduro que padecen enfermedad discal degenerativa (EDD) en la columna lumbar en uno o dos niveles contiguos de L2 a S1.


Para más informaciones, consulte a la Técnica quirúrgica Twin Peaks OLIF.



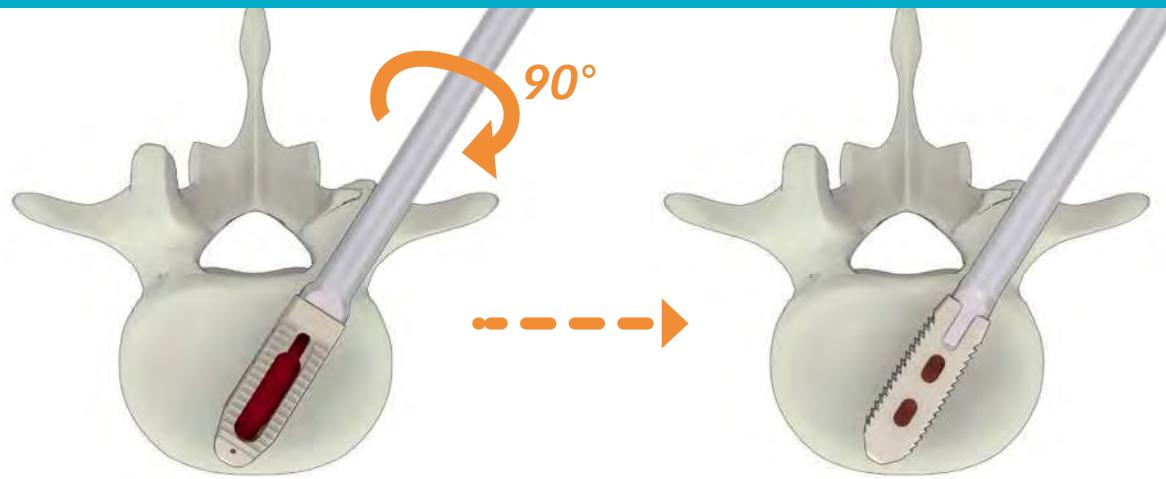

With rotation feature

Avec la caractéristique de rotation
Con característica de rotación

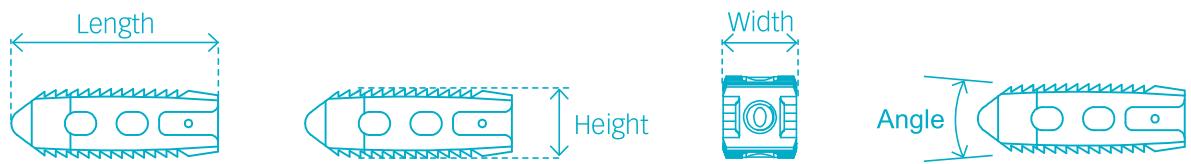

Twin Peaks oblique lumbar cage Twin Peaks cage lombaire oblique Twin peaks caja lumbar oblicua

Length 28

Height	Width	Angle	Rotation
		0°	
7	10	TP107280	-
8	10	TP108280	-
9	10	TP109280	-
10	10	TP1010280	-
11	10	TP1011280	✓
12	10	TP1012280	✓
13	10	TP10113280	✓
14	10	TP1014280*	✓

Length 32

Height	Width	Angle	Rotation
		0°	
7	10	TP107320	-
8	10	TP108320	-
9	10	TP109320	-
10	10	TP1010320	-
11	10	TP1011320	✓
12	10	TP1012320	✓
13	10	TP1013320	✓
14	10	TP1014320*	✓



Materials:

- PEEK OPTIMA® by Invibio®
- Radio-opaque markers: Tantalum.

All dimensions are measured in millimeter

*On request, delivery time not guaranteed

Matériaux :

- PEEK-OPTIMA® par Invibio®
- Marqueurs radio-opaques : Tantale

Toutes les dimensions sont mesurées en millimètres.

*Sur demande, délai de livraison non garanti

Material :


- PEEK OPTIMA® por Invibio®
- Marcadores radiopacos: Tántalo.

Las dimensiones se mide en milímetros

*Bajo pedido, plazo de entrega no garantizado

Twin Peaks by SPINeway

PLIF Bullet Shaped

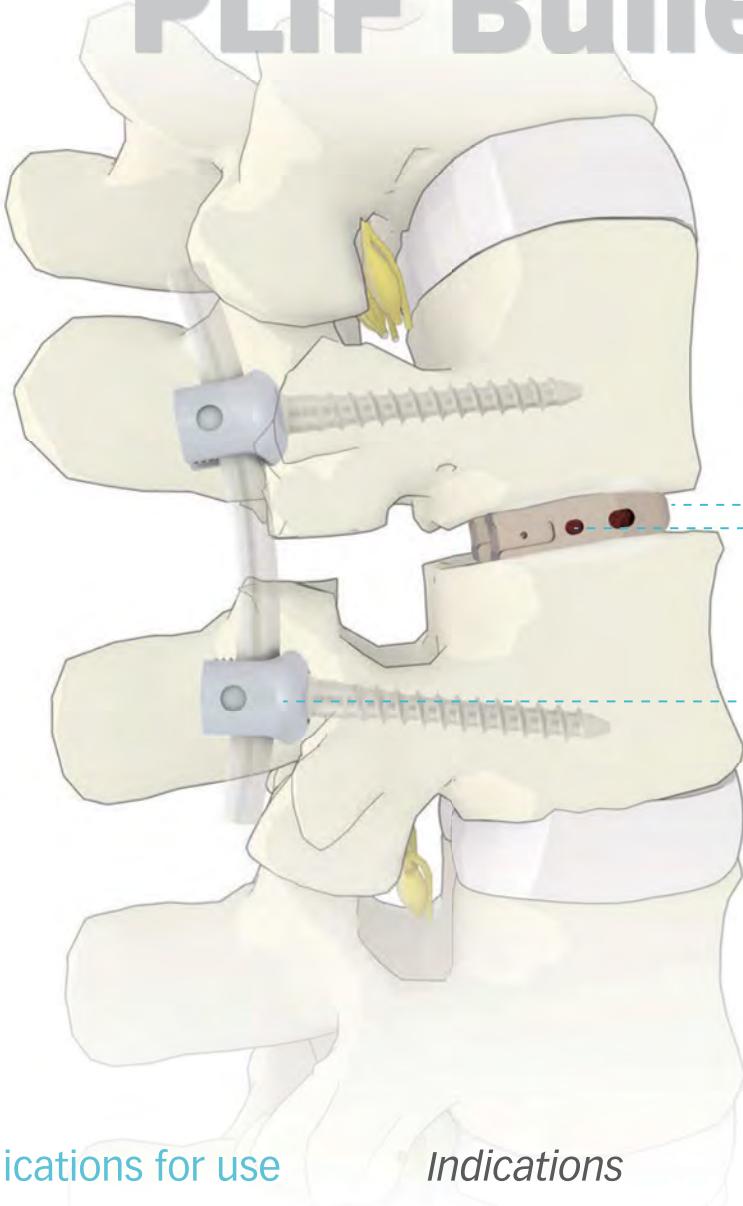

Indications for use

Intervertebral body fusion procedures in skeletally mature patients with degenerative disc disease (DDD) of the lumbar spine at one or two contiguous levels from L2-S1.

For more information, please consult the Twin Peaks PLIF BS Surgical technique.

Indications

Interventions de fusion intervertébrale chez des patients dont le squelette a atteint la maturité, souffrant de discopathies dégénératives (DDD) de la colonne vertébrale, à un ou deux niveaux contigus, de L2 à S1.

Pour plus d'informations, merci de vous reporter à la technique opératoire Twin Peaks PLIF BS.



Lumbar cage PLIF Bullet Shaped
Cage lombaire PLIF Bullet Shaped
Caja lumbar PLIF Bullet Shaped



Sonora or Neve

OUTSIDE USA:
sonora : calcium phosphate ceramic granules
neve : hydroxyapatite nanoparticle gel

HORS ÉTATS-UNIS :
sonora : Granules de céramique de calcium phosphate
neve : Gel de nanoparticules d'hydroxyapatite.

FUERA DE EE.UU.:
sonora : Gránulos de cerámica de fosfato de calcio.
neve : Gel de nano partículas de hydroxiapatita


Mont Blanc - Pedicle screw system

Indicaciones de uso

Procedimientos de fusión de cuerpos intervertebrales en pacientes con esqueleto maduro que padecen enfermedad discal degenerativa (EDD) en la columna lumbar en uno o dos niveles contiguos de L2 a S1.


Para más informaciones, consulte a la Técnica quirúrgica Twin Peaks PLIF BS.



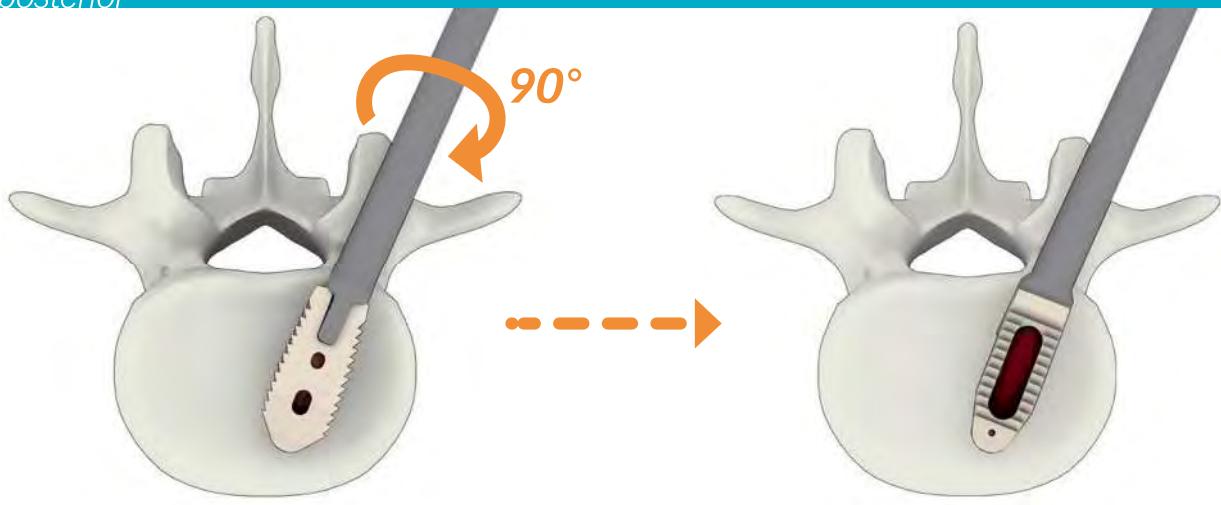

With rotation feature

Avec la caractéristique de rotation
Con característica de rotación

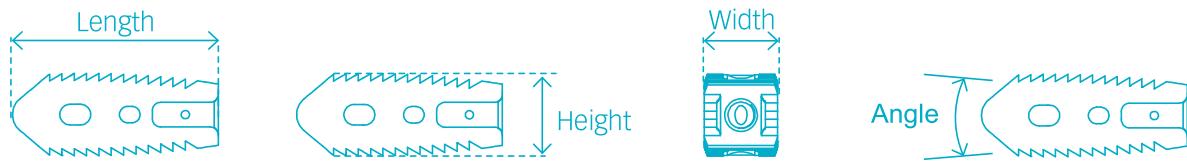

Twin Peaks PLIF BS lumbar cage Twin Peaks PLIF BS cage lombaire Twin peaks PLIF BS caja lumbar

Length 20

Height	Width	Angle		Rotation
		0°	4°	
7	8	TP1F7200	-	-
8	8	TP1F8200	TP1F8204	-
9	8	TP1F9200	TP1F9204	✓
10	9	TP1F10200	TP1F10204	✓
11	9	TP1F11200	TP1F11204	✓
12	10	TP1F12200	TP1F12204	✓
13	10	TP1F13200*	TP1F13204*	✓
14	10	TP1F14200*	TP1F14204*	✓

Length 25

Height	Width	Angle			Rotation
		0°	4°	8°	
7	8	TP1F7250	-	-	-
8	8	TP1F8250	TP1F8254	-	-
9	8	TP1F9250	TP1F9254	-	✓
10	9	TP1F10250	TP1F10254	TP1F10258	✓
11	9	TP1F11250	TP1F11254	TP1F11258	✓
12	10	TP1F12250	TP1F12254	TP1F12258	✓
13	10	TP1F13250*	TP1F13254*	TP1F13258*	✓
14	10	TP1F14250*	TP1F14254*	TP1F14258*	✓



Materials:

- PEEK OPTIMA® by Invibio®
- Radio-opaque markers: Tantalum.

All dimensions are measured in millimeter

*On request, delivery time not guaranteed

Matériaux :

- PEEK-OPTIMA® par Invibio®
- Marqueurs radio-opaques : Tantale

Toutes les dimensions sont mesurées en millimètres.

*Sur demande, délai de livraison non garanti

Material :

- PEEK OPTIMA® por Invibio®
- Marcadores radiopacos: Tántalo.

Las dimensiones se mide en milímetros

*Bajo pedido, plazo de entrega no garantizado